

# Agilent 385-ELSD Evaporative Light Scattering Detector For Low Molecular Weight Compounds

## Data Sheet



### Introduction

Evaporative light scattering detectors are ideal for detecting analytes with no UV chromophore as they do not rely on the optical properties of a compound. The Agilent 385-ELSD Evaporative Light Scattering Detector is the latest high performance ELSD from Agilent, benefitting from almost 20 years experience in the design and manufacture of evaporative light scattering detectors. The 385-ELSD is the only ELSD that delivers subambient operation, for unrivalled detection of thermally labile analytes. Designed for the analysis of all compounds, the 385-ELSD delivers evaporation down to 10 °C, providing maximum sensitivity for compounds with significant volatility below 30 °C. Programmable control of gas flow and temperature during an injection eliminates solvent gradient effects and maximizes response for improved accuracy. To detect everything you inject with high sensitivity, the 385-ELSD is the ELSD of choice for all applications.

### Key Benefits

- High sensitivity provides superb responses for all compounds, down to low nanogram levels.
- Subambient operation using a Peltier cooled evaporation tube delivers temperatures down to 10 °C, preventing degradation of the thermally labile compounds that other ELSDs cannot detect.
- Real-time control during an injection using programmable Dimension Software maintains maximum sensitivity throughout the run.
- Real-time gas programming using Dimension Software eliminates solvent enhancement effects during gradient elution, for excellent quantification.
- Low dispersion and high-speed data output rates are the perfect match for Fast LC applications.
- Superb reproducibility below 2% gives reliable and accurate results.



**Agilent Technologies**

## Key Benefits (Continued)

- Multivendor software control and data acquisition using Agilent ChemStation chromatography data system, and other vendors' interfaces, eliminates the need for an analog to digital converter.
- Rapid heating and cooling of the evaporator tube minimizes equilibration time.
- Full DMSO transparency ensures that responses from early eluting compounds are not hidden.
- Fully integrated with all Agilent analytical and preparative LC systems for the complete chromatographic solution.
- Complementary to LC/MS.

## System Details

The 385-ELSD delivers subambient evaporation down to 10 °C, providing maximum sensitivity for compounds with significant volatility below ambient temperature. The instrument benefits from fast data output rates and extremely low dispersion for fast LC, and delivers a universal response down to the low-nanogram range for truly representative analysis. Reproducibility is less than 2% for improved consistency of results. The 385-ELSD offers real time gas management that eliminates solvent effects to give a

constant response across a gradient. Control and digital data collection come as standard for multivendor platforms so there is no need for an analog to digital converter. On-the-fly adjustment of light source intensity can save time during a run. All this in the smallest footprint available. Being complementary to LC/MS, and offering unrivalled flexibility and sensitivity, the 385-ELSD is the ELSD of choice for the most demanding applications.

### Agilent's Family of Evaporative Light Scattering Detectors

Evaporative light scattering detection is the powerful alternative to RI and UV—inject it and detect it, right down to low nanogram levels. ELSDs provide a universal response independent of the optical properties of the analyte so there is no loss of important information.

You can use Agilent ELSDs for a wide range of analytical techniques, including LC (analytical and preparative), LC/MS, SFC, high throughput screening, GPC/SEC, TREF, and GPEC. The range of application areas is equally broad, encompassing pharmaceuticals, nutraceuticals, combinatorial libraries, carbohydrates, lipids, phospholipids, triglycerides, fatty acids, amino acids, polymers, and surfactants.

As the 385-ELSD delivers subambient evaporation down to 10 °C, it provides maximum sensitivity for compounds with significant volatility below 30 °C. For nonvolatile compounds, where temperatures of 100 °C or above are required, the Agilent 380-ELSD is the instrument of choice.

## Choose the Right Agilent ELSD for Your Needs

	Agilent 385-ELSD	Agilent 380-ELSD
HPLC analysis:		
Non-volatile compounds:	yes	yes
Semi-volatile compounds:	yes	yes
Highly volatile compounds:	yes	x
Ambient GPC analysis:	yes	yes
High temperature GPC analysis:	x	x


## Installation Qualification and Operation Qualification (IQ/OQ)

All Agilent ELSDs are rigorously tested to a high specification before they are shipped, and detailed IQ/OQ documentation is included with every unit. In addition, our detectors can be incorporated into any LC system, a complete Qualification Workbook is provided to help you.

## Uniform Mass Response

Agilent ELSDs are not dependent on a compound's optical properties so the ELSD provides a more uniform response than UV-VIS, making it the ideal detector for purity analysis or where calibration standards are not available.

Column: Agilent Polaris C18  
4.6 × 150 mm, 5 μm  
Eluent: Water/Acetonitrile 1:1  
Flow rate: 1.0 mL/min  
Injection volume: 10 μL  
Detector: Agilent 385-ELSD (neb = 30 °C,  
evap = 30 °C, gas = 1.4 SLM)

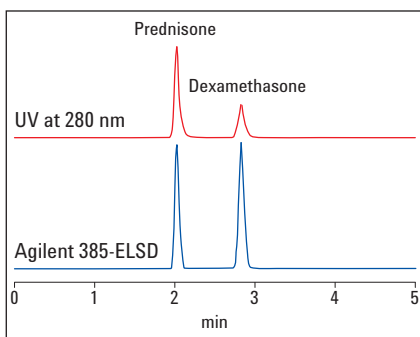

**Figure 1**  
The Agilent ELSD delivers a more uniform mass response than UV from a 1:1 mixture.

## Agilent ELSDs - Better by Design

Evaporative light scattering detection involves a three-stage process.

1. **Nebulization**—Using an inert gas stream to form a plume of uniformly sized droplets.
2. **Evaporation of the eluent**—Generating a plume of non-volatile solute particles.
3. **Optical detection**—Where the intensity of scattered light is proportional to the mass of solute passing through the optical chamber.


### Nebulization

Efficient nebulization using low gas flow rates is a feature of Agilent ELSD's. Independent nebulizer temperature control and digital gas flow control provide excellent stability and reproducibility. Baseline noise is minimized by the removal of any poorly nebulized eluent through a drain port.

### Evaporation

The nebulized stream passes through an independently temperature-controlled evaporator tube where solvent is removed at high temperature, leaving the less volatile solute particles behind.

The 385-ELSD features patented<sup>1</sup> gas flow control technology with a short evaporator tube that gives an extremely low swept volume for minimal peak dispersion. This provides maximum resolution from the separation, especially important for work with small columns.

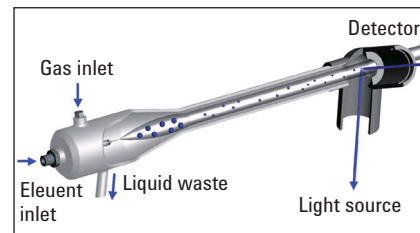

### Optical detection


The solute particles are detected as they pass through the optical chamber. The high power LED and advanced design of the electronics delivers maximum sensitivity.

<sup>1</sup> UK Patent 0304253.8, US Patent 6/0238744

## Fast LC

The excellent baseline stability across steep gradients and low dispersion characteristics combined with fast data output rates makes the 385-ELSD ideal for fast LC.

Sample: Tertiary aminols  
Column: C18 4 × 50 mm, 5 μm  
Eluent A: Water + 0.1% Formic acid  
Eluent B: Acetonitrile + 0.1% Formic acid  
Gradient: 5% to 95% B in 5 minutes  
Flow rate: 2.5 mL/min  
Injection volume: 10 μL  
Detector: Agilent 385-ELSD (neb = 40 °C, evap = 50 °C, gas = 1.5 SLM)

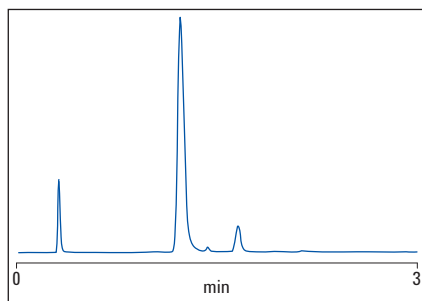


**Figure 2**  
The Agilent 385-ELSD provides a stable baseline even across steep, high speed gradients.

## Unrivalled Uniform Response across a Gradient

The 385-ELSD is unique in its ability to control gas flows during a run to produce a uniform detector response across a gradient. This real-time benefit offers an alternative approach to mobile phase compensation when quantifying unknowns under gradient conditions.

Column: Agilent Pursuit C18  
2.1 × 150 mm, 5 μm  
Eluent A: Water  
Eluent B: Acetonitrile  
Gradient: 5% to 95% B in 10 minutes  
Flow rate: 1.0 mL/min  
Injection volume: 10 μL (every minute)  
Detector: Agilent 385-ELSD (neb = 30 °C, evap = 30 °C)

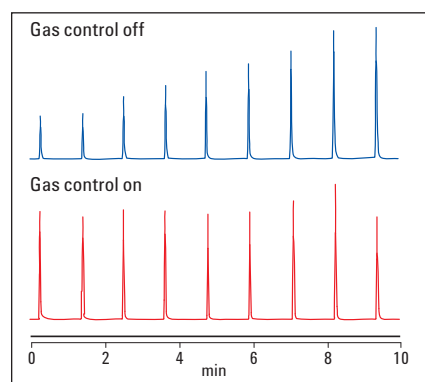


**Figure 3**  
Real-time gas control using Dimension Software provides unrivalled uniformity across a gradient.

## Sub-ambient ELSD

The Agilent 385-ELSD's unique cooled evaporation zone provides sub-ambient operation to deliver unrivalled detection of low molecular weight compounds not seen by other evaporative light scattering detectors.

Sample: Parabens  
Column: Agilent Pursuit C18  
2.1 × 150 mm, 5 μm  
Eluent A: Water  
Eluent B: Acetonitrile  
Gradient: 5% to 70% B in 5 minutes;  
70% to 95% B in 2 minutes  
Flow rate: 0.2 mL/min  
Injection volume: 10 μL  
Detector: Agilent 385-ELSD (neb = 30 °C, evap as shown, gas = 1.4 SLM)

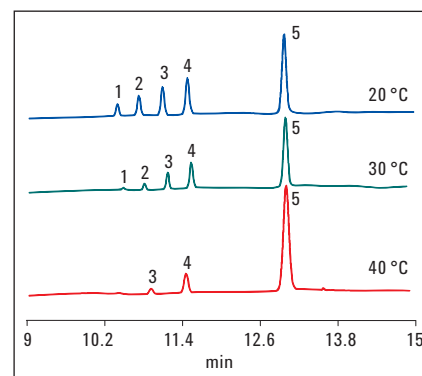


**Figure 4**  
Improved detection of parabens using sub-ambient ELSD with the Agilent 385-ELSD (parabens mixture injected at 100 ng except heptyl at 160 ng).

## Superb RSD

Excellent reproducibility below 2% gives reliable and accurate results. You can have complete confidence in your data.


Column: Agilent Pursuit C18  
150 × 4.6 mm, 5 μm  
Eluent: Water/Acetonitrile 40:60  
Flow rate: 1.0 mL/min  
Injection volume: 10 μL  
Detector: Agilent 385-ELSD (neb = 40 °C,  
evap = 40 °C, gas = 1.4 SLM)

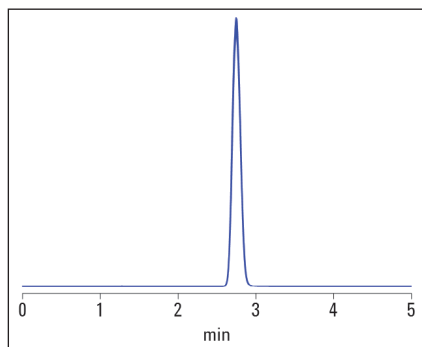

**Figure 5**  
Fifty caffeine injections produce an RSD of 1.27%, demonstrating the superb reproducibility of the Agilent 385-ELSD.

## Fast Temperature Switching

For higher throughput of samples, the unique 385-ELSD features rapid temperature equilibration. The detector cools from 50 °C to 30 °C, and *vice versa*, in just over five minutes. In addition to the enhanced detection of semivolatile compounds, the temperature controlled evaporator tube on the Agilent 385-ELSD allows the user to rapidly change between temperature programs.

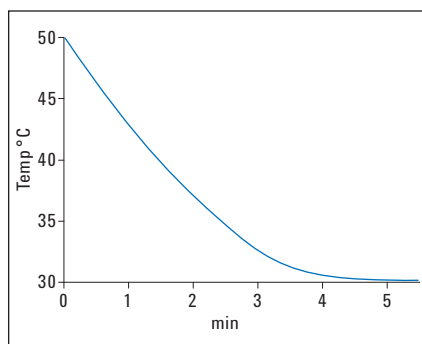


**Figure 6**  
Fast temperature equilibration with the Agilent 385-ELSD.

## DMSO Transparency for High Throughput Screening

The vast majority of combinatorial libraries screened by high throughput methods are stored in dimethylsulfoxide (DMSO). UV and mass spectrometry will miss potential drug compounds that have no UV chromophore, so ELSD is commonly used. However, at the low evaporator temperatures required to detect volatile components, the presence of DMSO in the sample can mask the response of early eluting compounds. In the 385-ELSD, the addition of a carefully controlled stream of gas to the evaporation step enables complete removal of the DMSO to take place without increasing the operating temperature.



Sample: 2 mg/mL in DMSO  
Column: 4.6 × 150 mm, 5 μm  
Eluent A: 0.1% HFBA in Water  
Eluent B: 0.1% HFBA in Acetonitrile  
Gradient: 5% to 30% B in 10 minutes,  
30% to 80 % B in 5 minutes  
Flow rate: 1.0 mL/min  
Injection volume: 20 μL  
Detector: Agilent 385-ELSD (neb = 25 °C,  
evap = 25 °C, gas as shown)

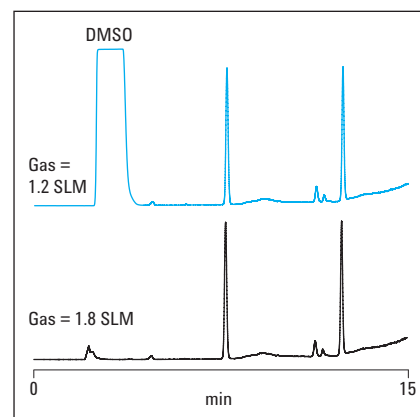

**Figure 7**  
Increasing gas flow on the Agilent 385-ELSD gives DMSO transparency.

## Adding Value to LC/MS

The 385-ELSD is fully complementary to LC/MS. The instrument can provide better data and support information for compounds that do not perform well on mass spectrometers, such as haloperidol, enhancing the value of your LC/MS system.

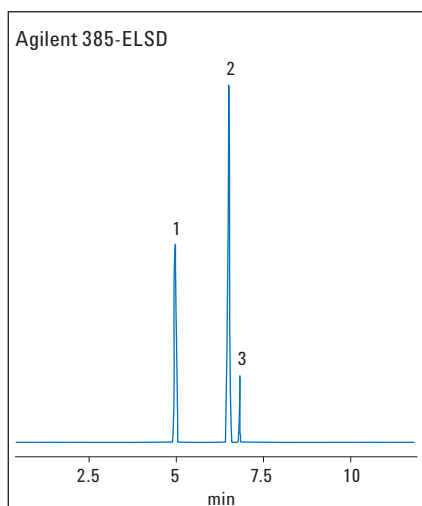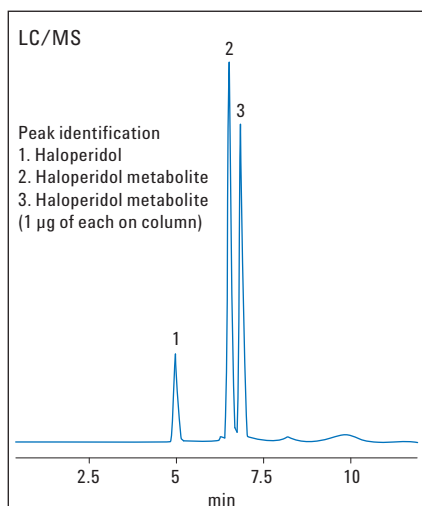

**Figure 8**  
 Coupling the Agilent 385-ELSD with LC/MS reveals much greater detail in the analysis of haloperidol and its metabolites.

Use of the sophisticated 385-ELSD software ensures improved detection of compounds not normally amenable to LC/MS.

## Choosing Detector Settings

The unique patented gas flow operation of the Agilent ELSD makes it mobile phase independent. Instead, settings

are optimized according to the thermal sensitivity of compounds injected.

As a general rule, all solvents can be evaporated with nebulizer and evaporator temperatures at 30 °C and a gas flow of 1.6 SLM. This can be used as a starting point and adjustments made according to the sample injected (if necessary), see Table 1.

Compound class	Nebulizer temperature (°C)	Evaporator temperature (°C)	Gas flow (SLM)
Parabens	30	20	1.40
Vitamins	25	25	1.60
Phthalates	25	25	1.60
Analgesics	25	25	1.60
Sudan dyes	30	30	1.60
Glycerides	30	30	1.40
Alkaloids	40	40	1.40
Amino acids	50	50	1.60
Natural products	30	50	1.40
Antibiotics	40	85	1.20
Polar lipids	30	80	0.90
Carbohydrates	50	90	1.00

**Table 1**  
 Choosing detector settings.

## Technical Specifications

Agilent 385-ELSD		
Light source:	LED 480 nm (Class 1 LED Product)	
Detector:	Photomultiplier tube digital signal processing	
Temperature range:	Evaporator	OFF, 10–80 °C (1 °C increments)
	Nebulizer	OFF, 25–90 °C (1 °C increments)
Gas requirements:	Flow rate	0.9 SLM to 3.25 SLM at 25 °C with integrated controlled gas shut-off valve
	Pressure operating range	60–100 psi (4–6.7 bar)
Eluent flow rate:	0.2–5 mL/min	
Analogue output:	0–1 V FSD	
Digital output:	24 bit digital data, 10, 40, or 80 Hz	
Communication:	Serial (RS232) Remote start Input Remote A/Z Contact closure TTL	
Instrument operation:	Graphical vacuum fluorescent display with keypad Real-time control through ELSD Dimension Software 10 predefined methods	
PC operation (software):	Standalone control software utilities, Agilent ChemStation control software, Agilent EZChrom Elite control software	
Power requirements:	90/120V AC or 220/250V AC 50/60 Hz 2A max	
Detector status:	Standby, run	
Size:	Unpackaged	200 × 450 × 415 mm (w × d × h)
Weight:	Unpackaged	13 kg
Safety features:	Gas shut off valve, vapor and leak detection	

## Ordering Information

Product description	Part number
Agilent 385-ELSD (110 or 240 V) including ChemStation driver	G4261A
Agilent ELSD Dimension Software	PL0890-0375
Agilent ELSD Driver for ChemStation	PL0890-0370

[www.agilent.com/chem/elsd](http://www.agilent.com/chem/elsd)

This information subject to change without notice.

© Agilent Technologies, Inc., 2012  
Published in USA,  
May 1, 2012  
5990-8180EN



**Agilent Technologies**